

**FIG. 1**

The interface consists of several rectangular panels with rounded corners. On the left side, there are vertical tick marks labeled 124, 126, 120, and 122 from top to bottom. A large central panel contains the text <RECEIVED IMAGE>. To its right is a smaller panel displaying vital signs: Temperature: 98.6 and Pulse: 70 bpm. Further to the right is another vertical column with tick marks 120 and 122. Below these panels is a horizontal section labeled "Section 3. Gastro-Intestinal". It contains the question "Have you experienced nausea?" followed by two radio button options: a filled circle for "Yes" and an empty circle for "No". At the bottom of this section is the instruction "Note patient's coloring?" next to a color calibration bar.

124

126

120

122

<RECEIVED IMAGE>

Temperature: 98.6

Pulse: 70 bpm

Section 3. Gastro-Intestinal

"Have you experienced nausea?"


Yes

No


Note patient's coloring?

122


**FIG. 2**

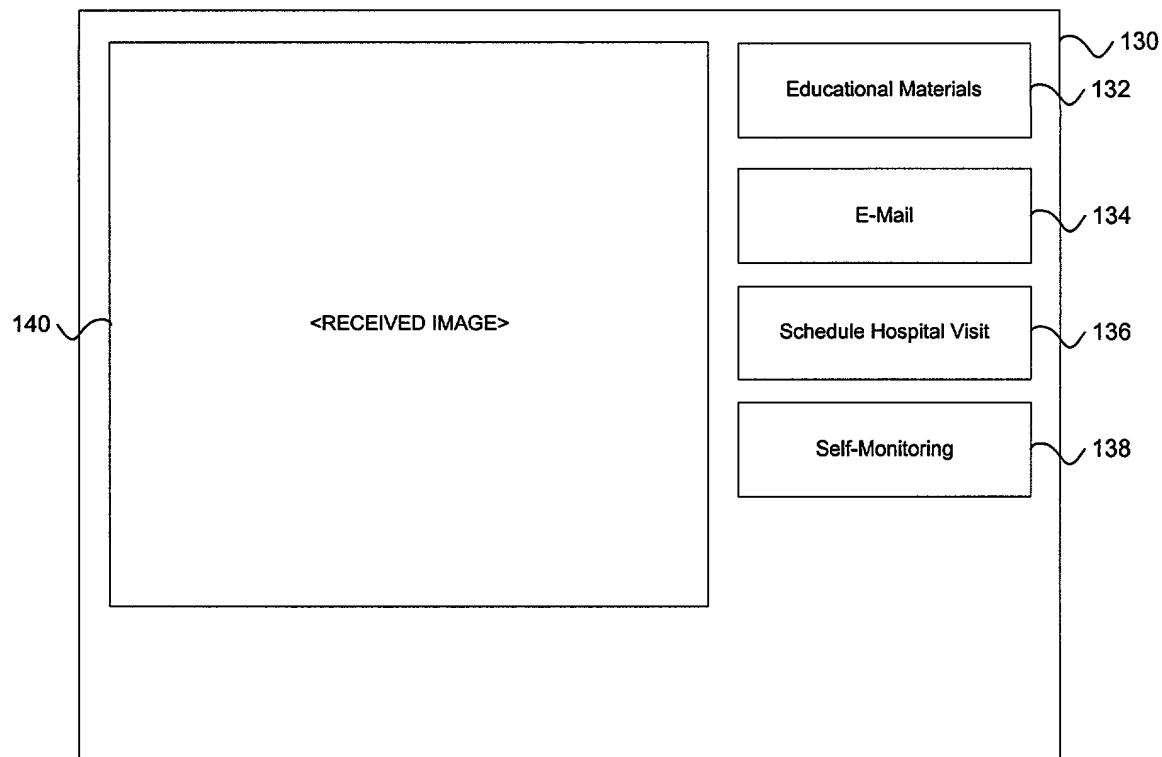


**FIG. 3**

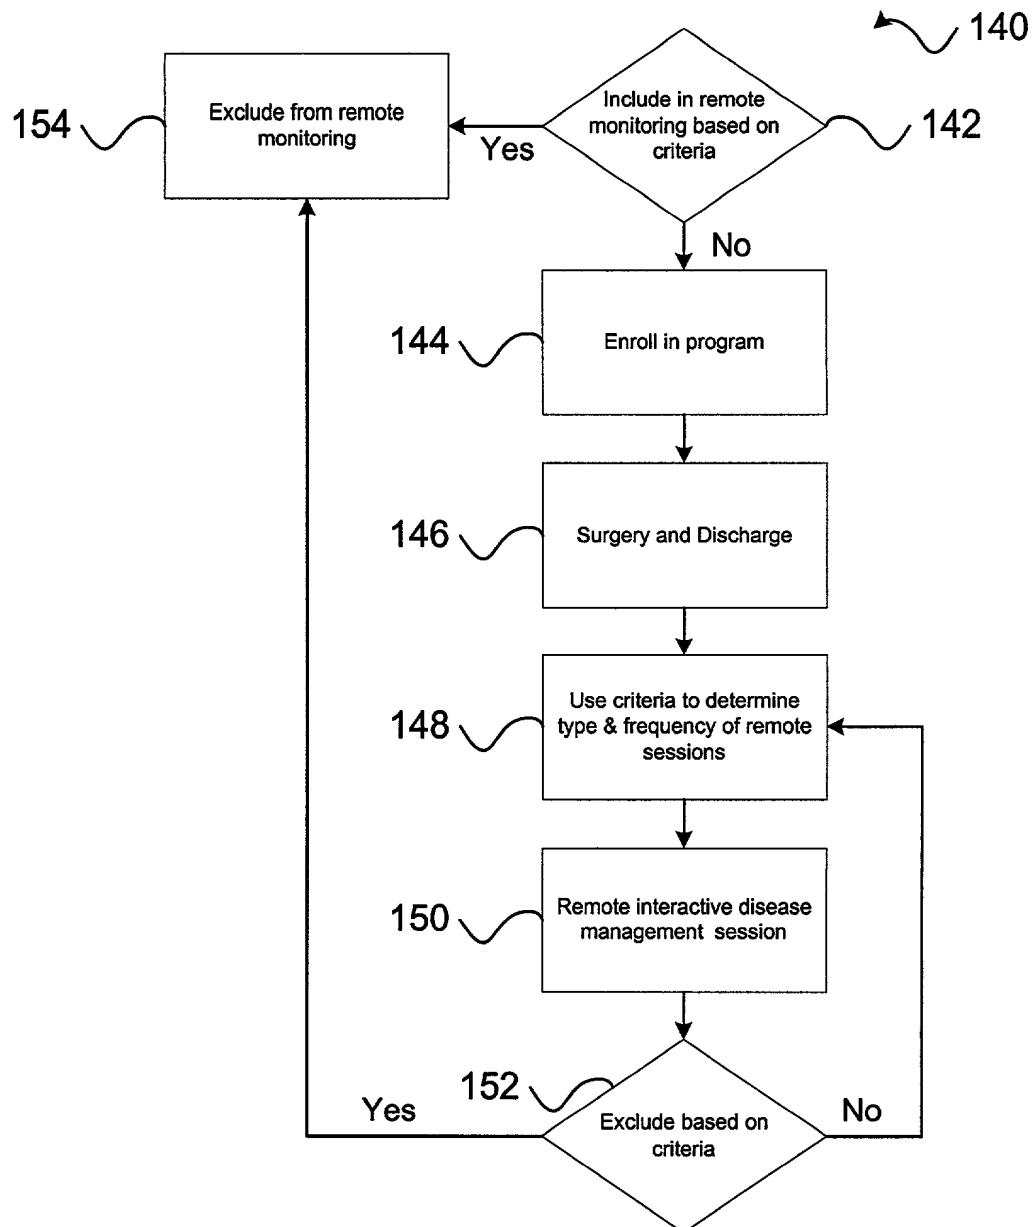**FIG. 4**

170  
172  
174  
176  
178

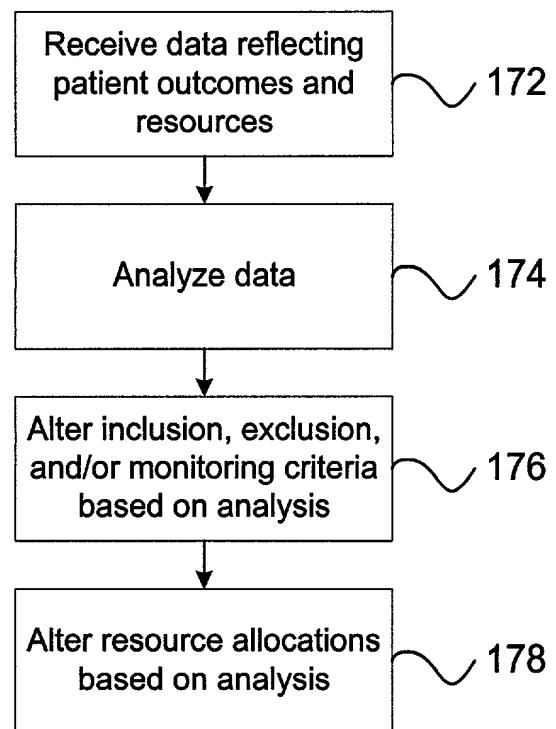

**FIG. 5**

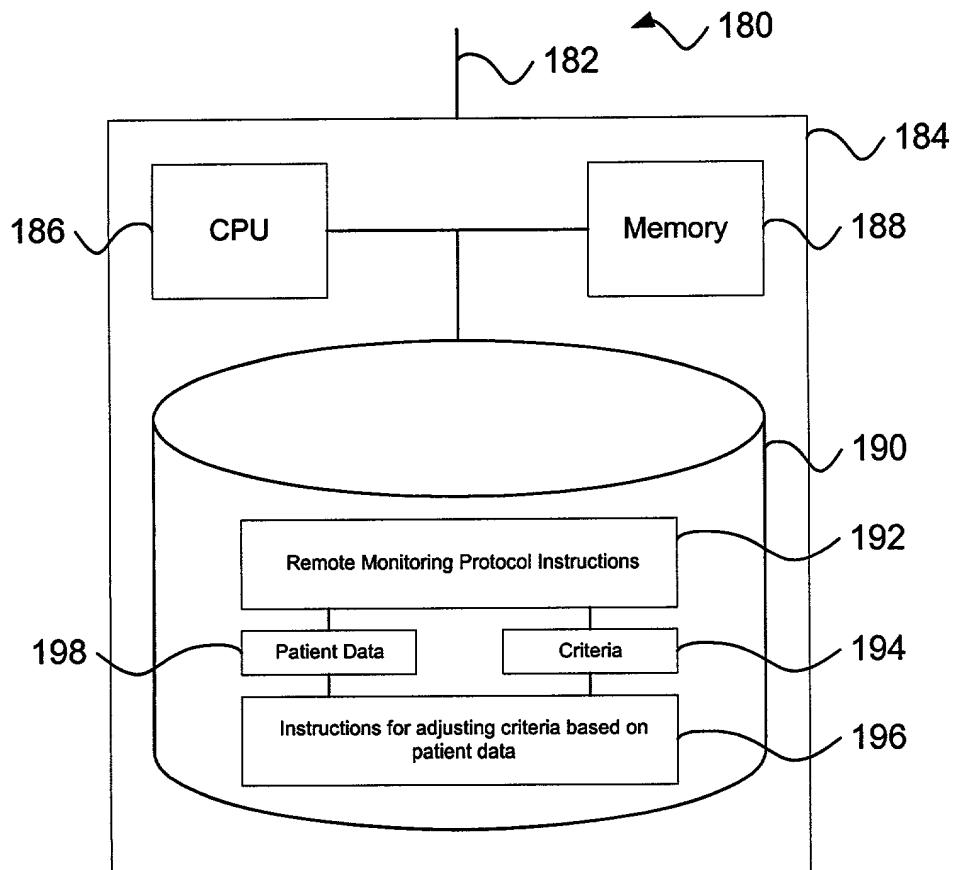

**FIG. 6**